



## Certificate of Compliance

Customer Name: Michigan Metrology, LLC    Date: 10/27/20

System Model:    NP Flex

System S/N: NPFLA-11-101

Next Certification Due: 10/27/23

This is to certify that the above system has been inspected, serviced and calibrated to ensure optimal operating performance.

The system calibration was conducted in accordance to the procedure outlined in the Bruker manual and was performed utilizing a certified standard which is traceable to NIST.

  
Thomas Coakley

Senior Field Service Engineer

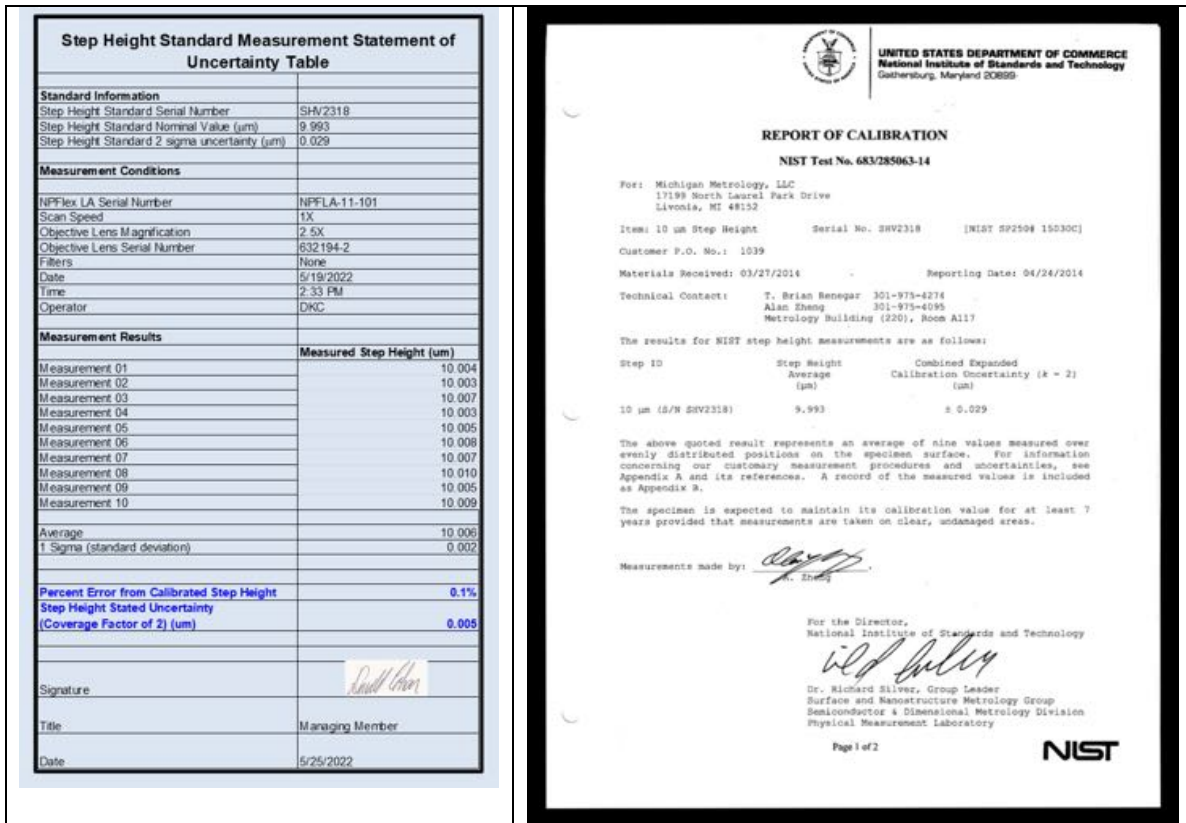


Figure 2. Measurement of NIST Traceable step standard is performed throughout the year for system verification and calibration.